

4200 Series

Getting Started Guide




4200 Series

Getting Started Guide

Cirris 4200 Series Testers combine thorough and flexible testing capabilities with a simple, touchscreen user interface for ease of operation. This guide will help the new user set up the tester and become familiar with its operation by working through the process of creating a test program and testing a cable.

For complete operating instructions, see the *4200 Series User Manual*, found on the USB flash drive supplied with the tester.

Symbols

| | |
|---|--|
|  | This symbol indicates that the 4250 tester produces high voltage and there is a risk of electric shock if safety warnings are not followed. |
|  | This symbol alerts the reader to a risk of personal injury. |
|  | This symbol indicates that a person using an electronically controlled medical device should not be permitted to perform high voltage testing. |

4250 Safety Warning



The 4250 tester is capable of performing high voltage Dielectric Withstand (DW) and Insulation Resistance (IR) testing. By design and function, the output of high voltage (hipot) testers presents a risk of electric shock. To mitigate this risk, 4250 testers limit current, high voltage energy and high voltage charge to levels below thresholds that define Hazardous Live or Dangerous in international standards IEC 61010-1 and EN 50191 respectively. However, operators can still receive a painful or startling shock when using any high voltage test equipment. Therefore, it's necessary to protect workers from exposure to high voltage.

Protecting workers begins with training. Operators should understand:

- Basic electricity including the fact that electric current will take any available path to ground, including through a person.
- How to use the test equipment and how to recognize when high voltage testing is being performed.
- Not to touch the product or test fixture hardware during high voltage testing.

A safe test station is an essential complement to training:

- Use a non-conductive work surface to avoid creating an unintended electrical path between high voltage and workers.
- Verify that the power outlet provides a properly wired, low impedance earth ground. The connection to earth ground is integral to the power cord supplied with the tester.
- Do not allow untrained workers to use high voltage test equipment.
- Isolate high voltage testing from untrained employees and post high voltage warning signs at the test station.

Medical Safety Warning



An individual wearing a cardiac pacemaker, an insulin pump, or any electronically-controlled medical device should NOT perform high voltage testing.

Intended Use



Cirris 4200 Series testers are designed for electrical testing and are intended to be used indoors, in a dry environment, at a temperature of 50-104 degrees Fahrenheit (10-40 degrees Celsius). High voltage Insulation Resistance measurements degrade at over 70% relative humidity.

No User-Serviceable Parts




The tester includes no user-serviceable parts. Attempting repairs or altering the tester in any way voids the warranty and may lead to an unsafe condition. Contact Cirris Technical Support for assistance if needed.


Unpacking

The package in which the tester was shipped should have included the following items:


- 4200 or 4250 Tester

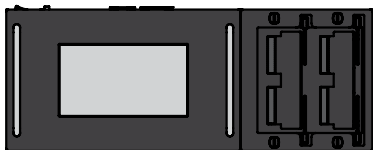


- USB Cable

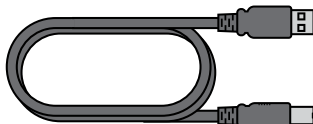


- Power Cable

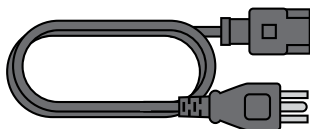

- Probe

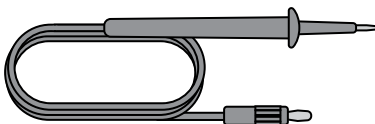

- Power Supply

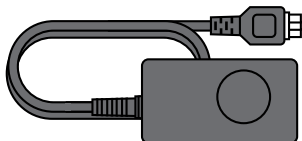

- WiFi Antenna



- Manual & software on USB Drive



You may have also received:


- Expansion Scanners
- Cirris Adapters
- Tilt Stand
- Performance Verification Kit
- Smart USB to Serial Printer Cable
- Label Printer

Hardware Setup

The tester includes 128 test points built into the base enclosure. It can be expanded to a maximum of 1024 test points using expansion scanners, each of which provides an additional 128 test points. If expansion scanners were included in the shipment, see the *4200 User Manual* for installation instructions.

After installing any expansion scanners, make the necessary connections on the back panel of the tester and power on the unit:

1. Connect the power cord to the tester.
2. Plug the power cord into a grounded outlet (surge protector recommended).
3. Connect the probe.
4. Press the power switch to turn on the tester.

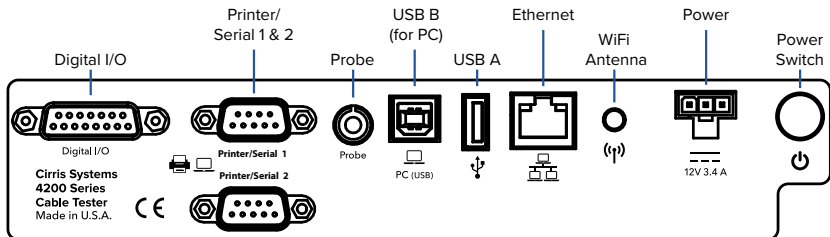

Networking

While it's not required to operate the tester, installing the included Cirris Hub software on a PC allows the tester to take advantage of its built-in Ethernet or WiFi networking capability to perform a variety of tasks including:


- Storing test programs on a network drive for easy backup of the files.
- Sharing test programs stored on a network drive or on a mapped cloud drive such as OneDrive, SharePoint, Google Drive, Dropbox etc.
- Printing reports to network printers.
- Saving reports as PDF or text files.
- Editing test programs using the Hub editor.
- Organizing testers with custom names and tracking calibration status and firmware version.
- Monitoring the current status of testers.

For more information on networking and the Cirris Hub, see the *Cirris Hub Manual* and the *4200 Series User Manual*.

System Settings

There are three system settings that should be changed or confirmed initially. On the **Main Menu**, select **System Settings**.

Several alternate languages are available for the 4200 Series user interface. To change the default language, select an alternate from the drop down box at the top of the screen.

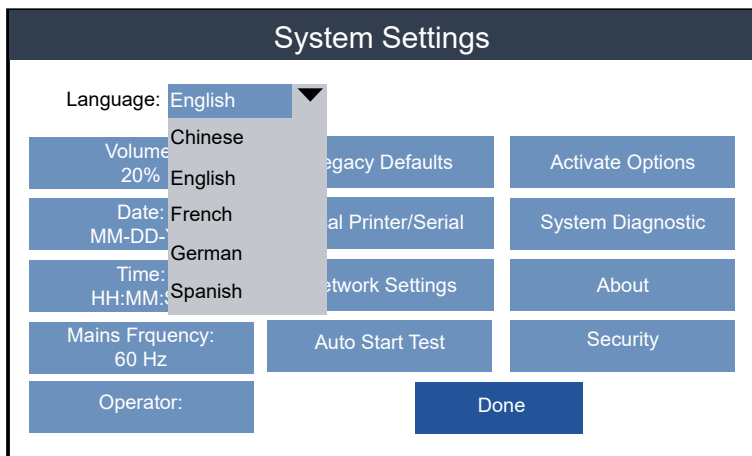

Tap the associated buttons to set the **Mains Frequency** and the current **Date** and **Time**, depending on the region of operation.

Tap **Done** when finished to return to the **Main Menu**.


Fixturing

The 4200 Series testers are compatible with the Cirris Adapter System which uses interchangeable adapters as the interface for connecting the tester to the Device Under Test (DUT). A large number of standard adapters providing a wide variety of connector types are available (a complete list of the standard adapters can be found on the Cirris web site). However, if the DUT includes connectors that have no direct adapter mates, test cables can be used to connect the connector on a standard Cirris adapter to the DUT connector. Your Cirris sales representative can also provide pricing for custom adapters.

Adapters are available in three sizes. Single-high adapters plug into one receptacle on the tester (e.g. J1). Double-high adapters plug into two vertically-adjacent receptacles (e.g. J1 & J2). Quad-high adapters plug into all four receptacles on the tester base or on an expansion scanner.

To attach an adapter to the tester:

1. Push the slidlocks, marked with red arrows in the graphic below, to the outward positions.
2. Set an adapter in one or more of the J1-J4 slots. Insert the adapter by pushing it to the left (toward the tester's screen) with steady, even pressure.
3. The adapter is fully seated when the slidlocks can be moved inward to hold the adapter in place. Using the slidlocks will reduce the stress on the adapter pins and on the tester's receptacles increasing the lifespan of both.

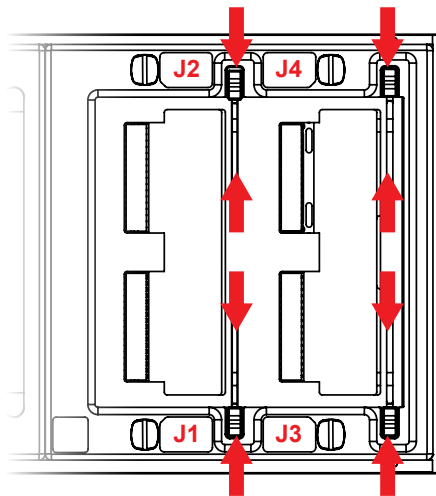


Create New Test Program

Before a cable can be tested, a test program must be created. This is most often accomplished by using the tester's capability to "learn" a sample product. Once a test program has been created, it can be saved and then loaded when needed to test subsequent batches of the same product.


To create a test program using the Learn feature:

1. Install the appropriate adapters.
2. From the tester's **Main Menu**, press **Create New**.

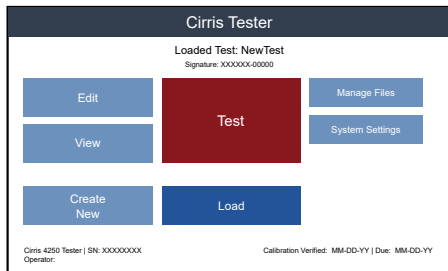


3. Press **Edit Learn Settings** to adjust settings per the cable specifications.

Note: Edited learn settings will be saved as the default for subsequent program learning.

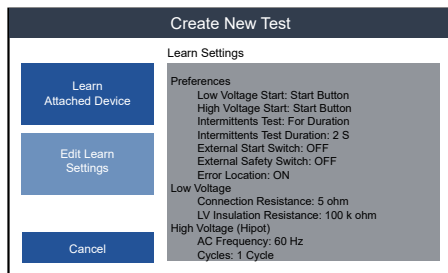

4. Using the category options on the left side of the screen, adjust the learn settings to match your cable's specifications.

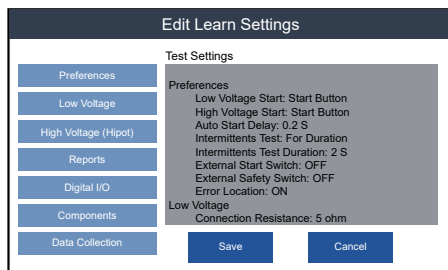

Learn Settings

Preferences:

Set the low voltage start condition (and high voltage start condition if using a 4250 tester). Set the desired Intermittents Test parameters and decide whether to prompt the operator to enter a Lot ID.

Low Voltage:

Set the maximum acceptable connection resistance and the minimum insulation (isolation) resistance.

High Voltage (Hipot) on 4250 only:

Set hipot voltage, minimum insulation resistance, and dwell time. If needed, **Advanced Settings** can be accessed to adjust dielectric withstand test parameters separately.

Reports:

Select reports/labels and configure print settings.

Digital I/O:

The testing process can be automated by including Digital I/O in the test program. See the *4200 User Manual* for more information.

Components:

Designate which components, if any, are included in the DUT. Options include resistors, capacitors, diodes and twisted pairs. Adding a 4-Wire component will instruct the tester to identify 4-Wire pairs in the test fixture before learning the DUT.

Perform a Learn

1. After making any required changes to the Learn Settings, select **Save** to return to the **Create New Test** screen. Attach the sample DUT and press **Learn Attached Device**. The tester will scan the DUT and create a test program.

The screenshot shows the 'Create New Test' interface. On the left, there are three buttons: 'Learn Attached Device' (highlighted in blue), 'Edit Learn Settings', and 'Cancel'. On the right, the 'Learn Settings' panel is visible, containing the following information:

- Learn Settings**
- Preferences**
 - Low Voltage Start: Start Button
 - High Voltage Start: Start Button
 - Intermittents Test: For Duration
 - Intermittents Test Duration: 2 S
 - External Start Switch: OFF
 - External Safety Switch: OFF
 - Error Location: ON
- Low Voltage**
 - Connection Resistance: 5 ohm
 - LV Insulation Resistance: 100 k ohm
- High Voltage (Hipot)**
 - AC Frequency: 60 Hz
 - Cycles: 1 Cycle

2. After the learn is complete, the tester will display the test program on the **Verify and Save Learned Test Program** screen. Review the program and verify that the settings are correct and that the connections and any components match the documentation for the DUT.

Saving Test Programs

After verifying that the test program is accurate, save the program using one of the two options:

Save

Selecting **Save**, stores the program in the default location using the filename “NewTest.wir.” The next time a test program is learned, selecting **Save** would repeat the process overwriting the test program previously saved with the “NewTest.wir” filename.


Save As...

Selecting **Save As...**, allows the user to select a storage location and a name for the test program.

1. Navigate to a location within the directory to save the test program. If using the Cirris Hub Software, saving files to the network location (F:) will allow other networked testers to use the test program also.

Note: *The selected location will be the default the next time a test program is saved or loaded.*

2. To name the new test program, select **New...**, enter a name for the program, and press **Done**.

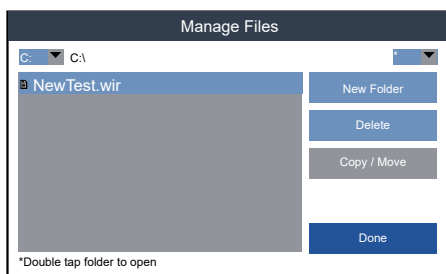



Load a Test Program

From the **Main Menu**, press **Load**. Navigate to the desired directory by selecting a drive from the top left drop-down box. Open a folder by tapping on it twice. To go back, double-tap the folder with the trailing two dots (..).

When the desired test program has been located, select it and press **Load**. The name of the loaded test program will appear at the top of the **Main Menu**.

Test

1. From the **Main Menu**, check that the correct test program is loaded and press **Test**.
2. Depending on the Start Condition, either attach a cable to start the test automatically or attach a cable and press **Start Test**.
3. The low voltage testing is initiated and may take less than a second to complete.
4. For 4250 testers, if the low voltage portion of the test passes, the high voltage (hipot) test window will open and the test will begin depending on the start condition. If the low voltage portion of the test fails, the test will terminate.
5. If an intermittents test was programmed, it will begin after the test passes on a 4200 tester and after the high voltage test passes on a 4250 (if a hipot test was programmed). Flex the cable to check for intermittent errors. The test will end depending on the intermittents test settings.
6. If the test passed, the header will turn green and display “Passed.” If the test failed, the header will turn red and display “Failed” and the error details will appear in the test window.

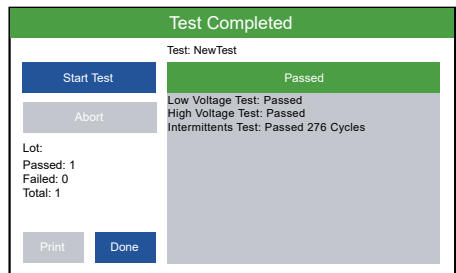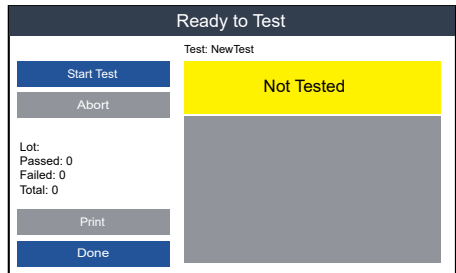

Common Errors

Open Errors: A gap exists in an intended electrical path.

Short: Unintended contact between two or more conductors.

Miswire: A conductor is terminated to an incorrect contact.

For more information on errors, refer to the *4200 Series User Manual*.

Finishing a Test

When the test is complete, disconnect the DUT from the tester. The test screen will reset and be ready for the operator to connect another cable, or press **Done** to return to the **Main Menu**.

If a report was added to the test, it will print automatically when the DUT is disconnected or the operator can press **Print**.

Help / Support

For assistance with your Cirris test system:

- See the *4200 Series User Manual* provided on the USB flash drive supplied with the tester.
- Visit www.cirris.com/learning-center to access articles about Cirris products and a variety of testing-related subjects.
- In the United States, contact technical support at TechSupport@cirris.com or by telephone at 1-801-973-4600.
- Outside the United States, visit www.cirris.com to find your Cirris sales and support representative.

The logo for Cirris, Inc. features the word "CIRRIS" in a bold, red, serif font. A registered trademark symbol (®) is positioned at the top right of the letter "S".

Cirris, Inc.
401 North 5600 West
Salt Lake City, UT 84116
USA
1-801-973-4600
www.cirris.com

Version 2021.31